


Mass Spectrum

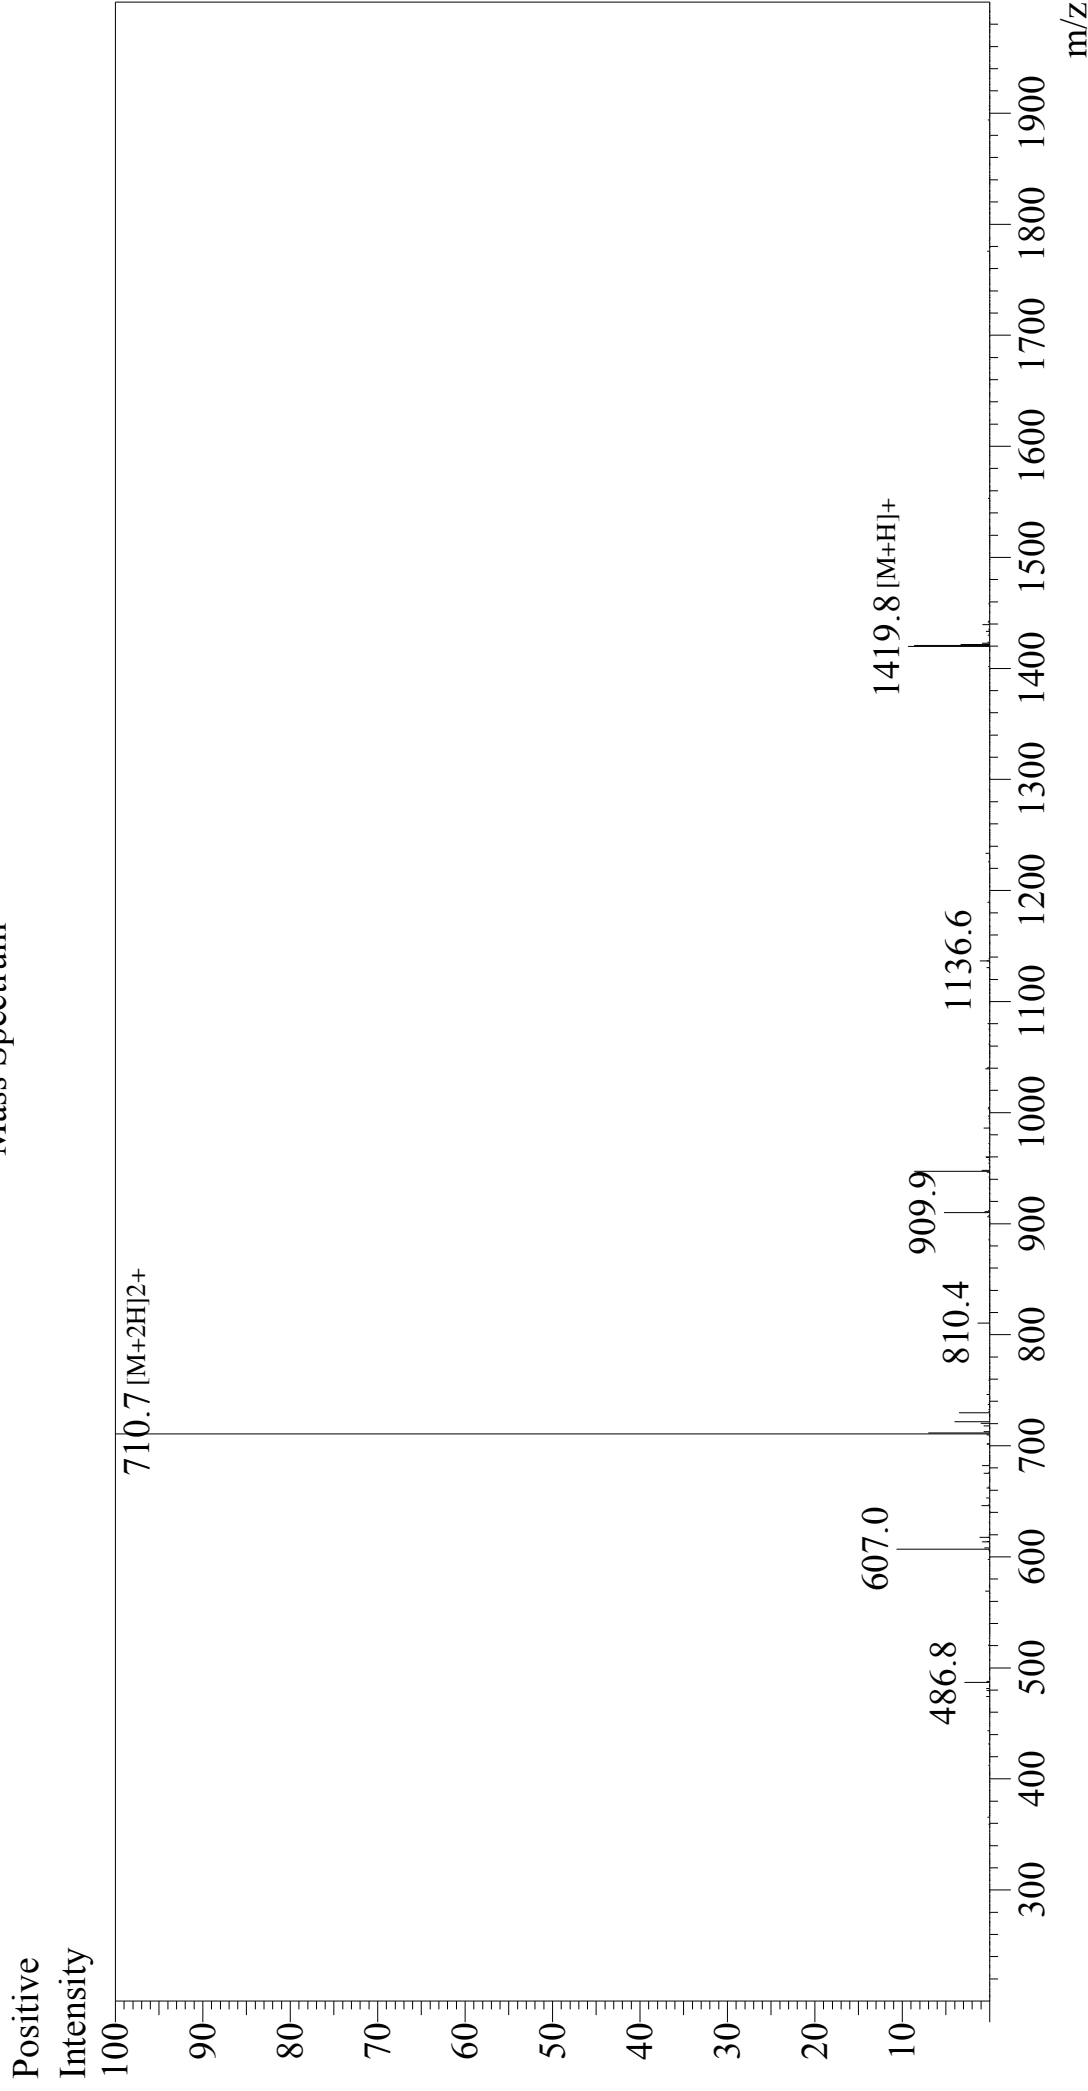

Sample Information

Month-Day Processed : 06/21/25
Time Processed : 20:13:13
Injection Volume : 0.2
Sample Name : BPC-157
Sample ID : U3398KSTG0-9
Theoretical MW : 1419.56
Observed MW : 1419.4

Interface : ESI
Nebulizing Gas Flow : 1.5 L/min
CDL Temp : 250
Block Temp : 200
Equipment : ZJ22010150
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H₂O/50% MeOH