

Sample Name :Semaglutide (Ozempic Active Ingredient)
Sample ID :U3398KSTG0-6
Time Processed :13:11:20
Month-Day-Year Processed :07/18/2025

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
10.00	Pumps	B.Conc	35
35.00	Pumps	B.Conc	95
37.00	Pumps	B.Conc	95
37.01	Pumps	B.Conc	5
45.00	Pumps	B.Conc	5
45.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm
Equipment: ZJ21010026

<Chromatogram>

mV

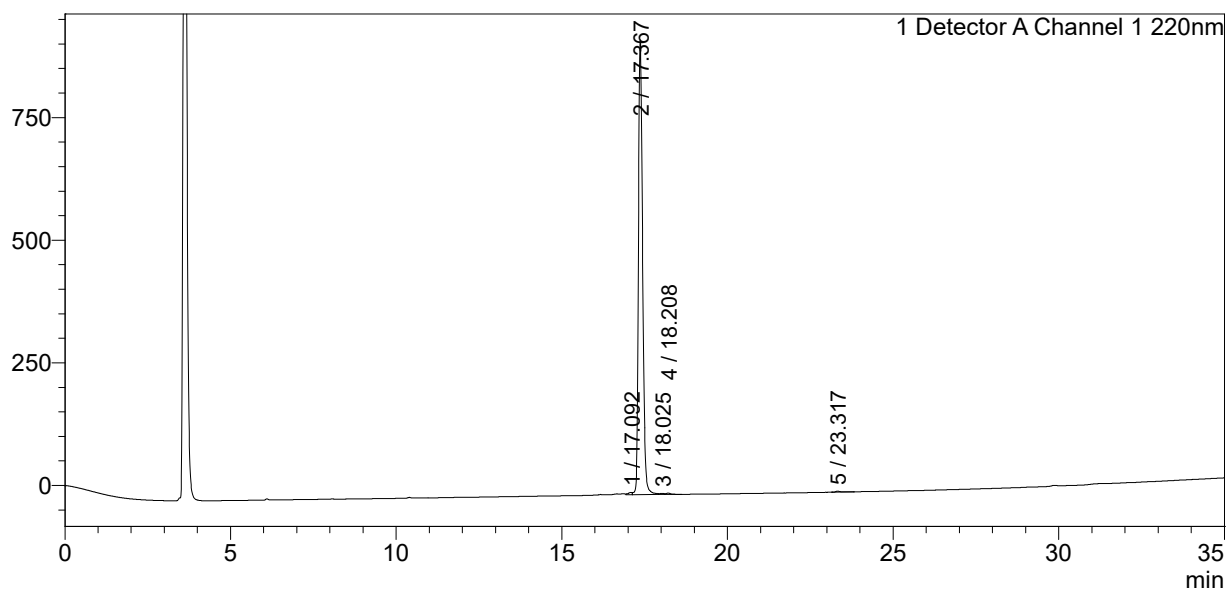

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	17.092	35841	4374	0.432
2	17.367	8184003	927234	98.749
3	18.025	21275	2220	0.257
4	18.208	25864	2565	0.312
5	23.317	20735	1930	0.250
Total		8287718	938323	100.000