


Mass Spectrum

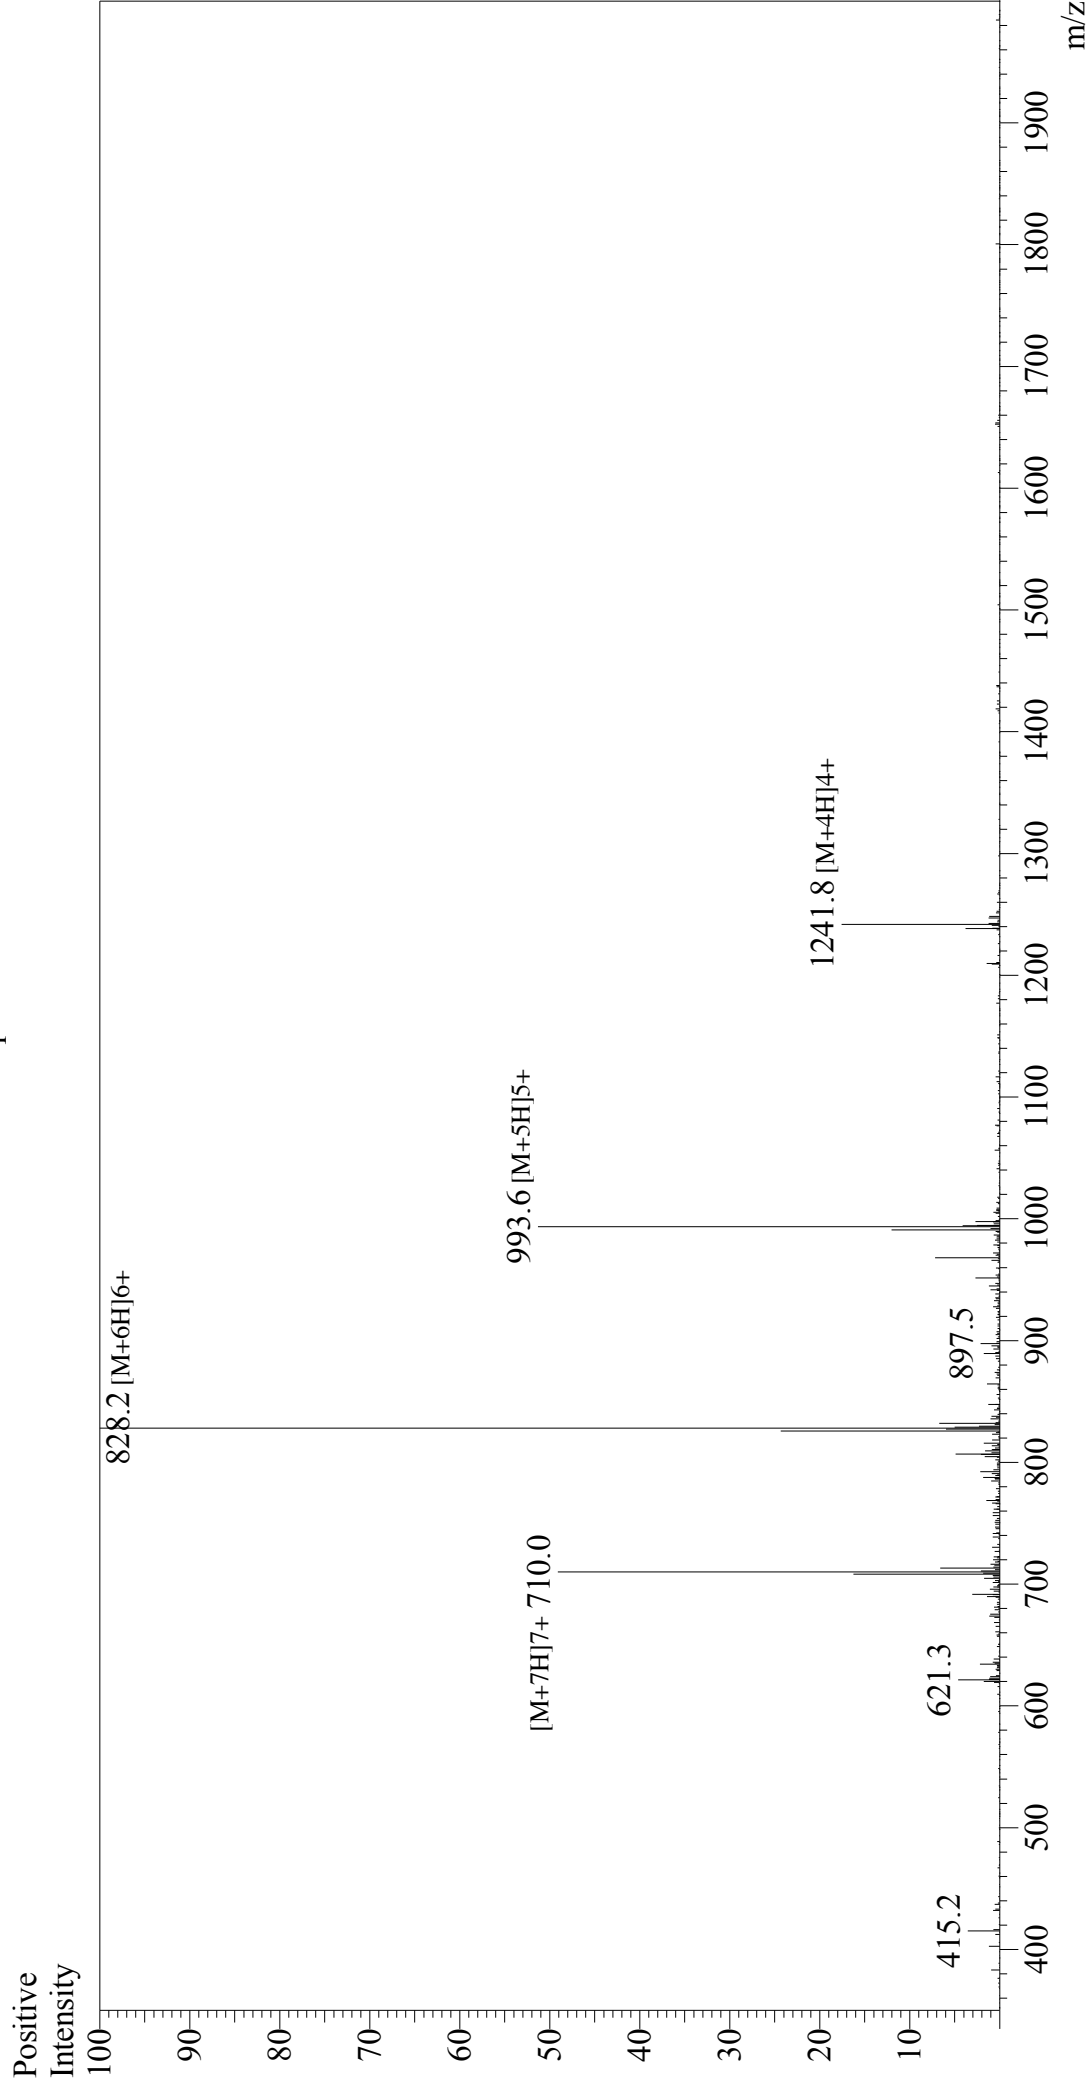

Sample Information

Month-Day Processed : 07/29/25
 Time Processed : 10:30:45
 Injection Volume : 0.2
 Sample Name : TB-500 (Thymosin Beta-4 Fragment)
 Sample ID : U3398KSTG0-10
 Theoretical MW : 4963.51
 Observed MW : 4963.2

Interface

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment

Equipment : ZJ21010035
 Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50%H₂O/50%MeOH